


## Test Report P-30

Accuracy\* (10 ... 60 °C): 0.1 %  
 Pressure range: 0 ... 1 bar rel.  
 Signal: 0 ... 10 V  
 ProductNo. (P#): 38341505  
 Serial No. (S#): 2252918


### Results

Standard bar	Accuracy *	
	V	%
0.000	-0.001	-0.007
0.250	2.498	-0.015
0.500	4.998	-0.023
0.750	7.497	-0.026
1.000	9.998	-0.021

\* Including non-linearity, hysteresis, zero point and full scale error (corresponds to error of measurement per IEC 61298-2).

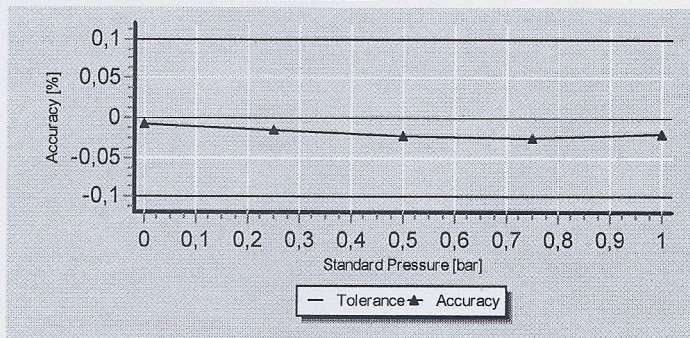

# SOUTH AFRICAN NATIONAL ACCREDITATION SYSTEM



WIKA Instruments (Pty) Ltd - South Africa

## CALIBRATION LABORATORY FOR PRESSURE MEASUREMENT



Certificate Number



### Certificate of Calibration

Calibration of a Transmitter

Manufacturer WIKA INSTRUMENTS

Type P-30  
Range 0 ... 1 bar

Serial number **2252918**  
Tag number n/a

Customer University Of Pretoria  
Roper street  
Room 3/57, Admin. Building  
Pretoria

South Africa

Order No. 0000327065

This calibration certificate documents the traceability to national standards and international standards, which realise the units of measurement according to the International System of Units (SI).

The South African National Accreditation System (SANAS) is a member of the International Laboratory Accreditation Committee (ILAC) for the Mutual Recognition Agreement. This arrangement allows for the mutual recognition of technical test and calibration data by the member's accreditation bodies worldwide. For more information on the MRA please consult [www.ilac.org](http://www.ilac.org)

The values in this certificate are correct at the time of calibration/certification. Subsequently the accuracy will depend on such factors as operating temperature, the care exercised in handling, frequency of use and its use under conditions other than specified by the manufacturer and/or conditions of calibration/certification. Recertification should be performed after a period that has been chosen by the user to ensure that the equipment's accuracy remains within the desired limits. The user is obliged to have the object recalibrated at these intervals.

The reported results are only valid for the object calibrated. Legal liability shall be limited to the cost of recalibration and or certification, but the applicant indemnifies WIKA INSTRUMENTS against any consequential or other loss.

Number of pages of the certificate 4

Date of calibration 14/08/2015  
**Recalibration Date As Per Customer August 2016**

*This calibration certificate may not be reproduced other than in full except with the permission of the issuing laboratory. Calibration certificates without Technical Signatory's signature and seal are not valid.*



Date of Issue

14/08/2015

SANAS Authorised Technical Signatory

Wellcome P.

Calibrated by

Calibration Technician

Mashileane T.

# WIKA Instruments (Pty) Ltd - South Africa



page 2 of 4: Date of calibration 14/08/2015

Certificate No. 

A 9913
SANAS
246

### Specification of device under test (DUT)

Pressure range	0 ... 1 bar
Method of measurement	Gauge pressure
Accuracy	0.1 % (of span )
Scale division	0.001 V
Output signal	0 ... 10 V

### Used auxillary instruments

Digital-Voltmeter	Keithley 2000 S# 0972922
Shunt (250 Ohm)	-

### Environmental conditions

Ambient Temperature in °C	20.8 +/- 1.6
Ambient pressure in mbar	837 +/- 0.59
Humidity %RH	28 +/- 5.7

### Place/ Location of calibration

WIKA Laboratory Johannesburg

### Reference Standard and test conditions

Working Standard (WS)	01783427DKD15-01
- Name	CPC 8000 S# Z80043C
- Range	-1 ... 1 bar
- Accuracy	0.0063 % referred to span
Pressure media	Oil
Reference height	Connection of obj.
Position during calibration	Vertical

### Extensions

### Calibration process

Method	Pressure-setting according to Reference
Cycle	B
Work instruction	LW-007 r6 & LW-012 r5

For calibration the following norm is used:

- DKD-R 6-1 Guideline for calibration of pressure gauges by German Calibration Service "Deutscher Kalibrier Dienst" (DKD) Edition 01/2003

WIKA Instruments (Pty) Ltd. Chilvers St.,  
Denver, 2094  
Johannesburg, South Africa  
PO Box 75225, Gardenview, 2047



Tel.: (011) 621 0000  
Fax: (011) 621 0059  
email: sales@wika.co.za

WIKA Instruments (Pty) Ltd - South Africa



page 3 of 4: Date of calibration 14/08/2015

Certificate No. A 9913  
SANAS  
246

**Results**

P <sub>e</sub> WS bar	calculated DUT bar		
	M 1	M 2	M 3
0.0000	0.0002	0.0003	0.0003
0.2000	0.2003	0.2003	0.2003
0.4000	0.4002	0.4002	0.4002
0.6000	0.6002	0.6002	0.6002
0.8000	0.8002	0.8002	0.8002
1.0000	1.0003	1.0003	1.0003

**Evaluation**

P <sub>e</sub> WS bar	Mean- value bar	Deviation bar	Repeat- ability b bar	Hysteresis bar	Uncertainty bar
0.0000	0.0000	0.0000	0.0000	0.0000	0.0001
0.2000	0.2000	0.0000	0.0000	0.0000	0.0001
0.4000	0.4000	0.0000	0.0000	0.0000	0.0001
0.6000	0.6000	0.0000	0.0000	0.0000	0.0001
0.8000	0.7999	-0.0001	0.0000	0.0000	0.0001
1.0000	1.0000	0.0000	-0.0001	0.0000	0.0001

The deviation must be subtracted algebraically from the device under test (DUT) reading to obtain the correct value.  
M1/M3 INDICATES RISING PRESSURE, M2/M4 INDICATES FALLING PRESSURE.

To convert in official-unit -kPa- use multiplier :100 kPa/bar

**NOTE: All readings entered on computer directly.**

WIKA Instruments (Pty) Ltd. Chilvers St.,  
Denver, 2094  
Johannesburg, South Africa  
PO Box 75225, Gardenview, 2047



Tel: (011) 621 0059  
Fax: (011) 621 0059  
email: sales@wika.co.za

# WIKA Instruments (Pty) Ltd - South Africa



page 4 of 4: Date of calibration 14/08/2015

Certificate No.


A 9913
SANAS
246

### Uncertainty

The reported expanded uncertainty of measurement is valid after a correction of the reading value with the systematical deviation (see table "evaluation").

The reported expanded uncertainty of measurement is stated as the standard uncertainty of measurement multiplied by the coverage factor  $k=2$ , which for a normal distribution corresponds to a coverage probability of 95,45%, the uncertainty of measurement has been estimated in accordance with the principles defined in the GUM, 'Guide to Uncertainty of Measurement, ISO, Geneva, 1993'.

### Graphic representation of the relative uncertainty

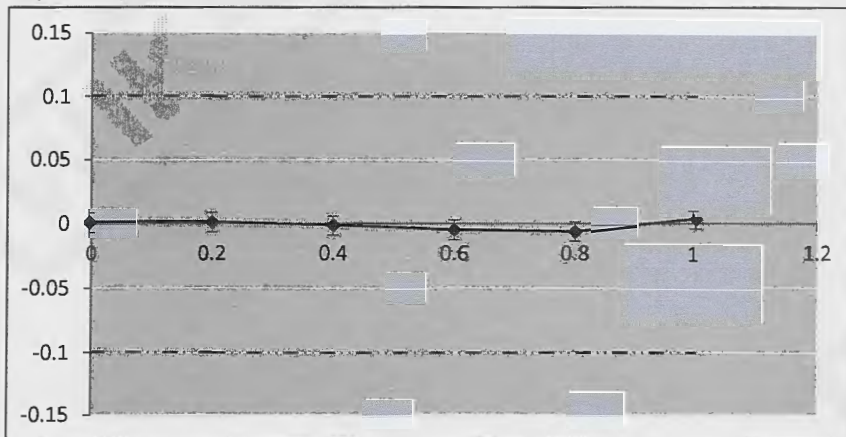

Legend	
X-axis	$P_e$ in bar
Y-axis	rel. uncertainty in %

### Accuracy of instrument

$\pm 0.00014$  bar =  $\pm 0.014$  % referred to span

### Label

The calibration object is labelled, which shows the number of this calibration certificate, serial/tag number and the date of calibration.

**END OF CERTIFICATE.**

The South African National Accreditation System (SANAS) is a member of the International Laboratory Accreditation Committee (ILAC) for the Mutual Recognition Agreement. This arrangement allows for the mutual recognition of technical test and calibration data by the member's accreditation bodies worldwide. For more information on the MRA please consult [www.ilac.org](http://www.ilac.org)



WIKA Instruments (Pty) Ltd - South Africa



ATTACHMENT 1 of 1 for certificate:

A 9913

Date of calibration

14/08/2015

Certificate No.

A 9913
SANAS
246

Listing of measured pressure-signals

pe bar	Output signal of transmitter V		
0.00	0.0024	0.0028	0.0027
0.20	2.0025	2.0026	2.0026
0.40	4.0024	4.0022	4.0024
0.60	6.0018	6.0021	6.0021
0.80	8.0019	8.0018	8.0018
1.00	10.0030	10.0028	10.0027

factory V

9.998

0.1 bar / V  
0 bar

